

Product Code

CNG050S290NCAAEZZZ

Serial ID

15330375

Order ID

10462906

Line Item

2.1 3

Customer Tag

22081332

Process

Process ID : 9.29601901

Process Time : 2022.02.24 6:58:46

Process Stand : SSF1E@SSCCL:1

Stand Uncertainty : +/-0.030%


Fluid : H2O

100% Rate : 38.6 KG/MIN

Pickoff : 1

Max Rate P/T : 41.84 PSIG/20.6 C

Detail

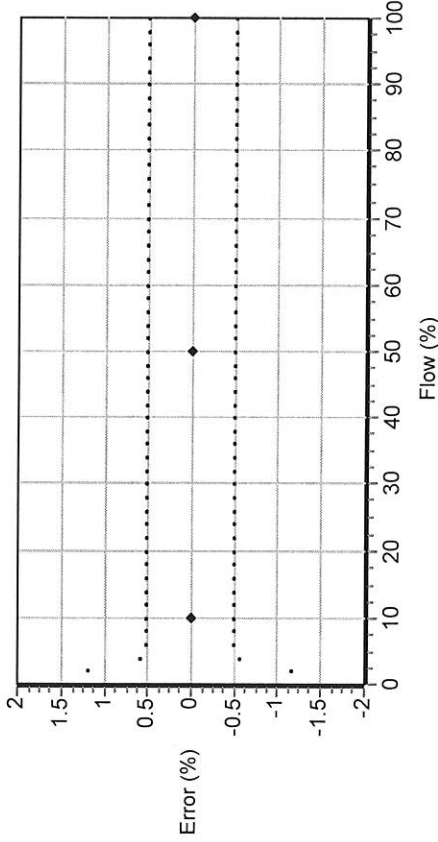

Results

Status : PASS

D1 : 0

D2 : 1

K1 : 4089.925

K2 : 4259.578

DT : 4.25

FD : 0

DTG : 0

DFQ1 : 0

DFQ2 : 0

FlowCal : 139.544.50

FFQ : 0

FTG : 0

DensCal : 04090042604.25

FCF : 139.54

FT : 4.5

Boyd/Kul

RAZVAN OCTAVIAN, COSMA

Technician

This certificate is produced by an electronic data system and is valid without signature.

Flow (%)	Flow Rate (kg/min)	Meter Total (kg)	Reference Total (kg)	Error (%)	Specification (±%)
100.0	38.6	38.23137	38.2328	-0.004	0.500
10.0	3.86	7.850983	7.851416	-0.006	0.500
50.0	19.3	19.73007	19.72973	0.002	0.500
100.0	38.6	38.19406	38.19975	-0.015	0.500

Product Code

CNG050S290NCAAEZZZ

2700I13ABAEZWW

PUCK700

Serial ID

15330375

3519996

26196747

Order ID

10462906

10462906

Line Item

2.1 3

2.33 3

Customer Tag

22081332

Process

Process ID : 1.36696390

Process Time : 2022.04.01 18:13:18

Process Stand : CONFIGURATION@SSCB

Sensor

D1 : 0

D2 : 1

DFQ1 : 0

DFQ2 : 0

DT : 4.25

DTG : 0

Dens PCF : 0

Density Meter Factor : 1

FCF : 139.54

FD : 0

FFQ : 0

FT : 4.5

FTG : 0

Flow PCP : 30

Flow PCF : 0

K1 : 4089.925

K2 : 4259.578

Mass Flow Meter Factor : 1

Volume Flow Meter Factor : 1

Units

Density Unit : G/CM3

GSV Flow Unit : SCFM

Mass Flow Unit : G/SEC

Pressure Unit : POUNDS/SQUARE INCH

Special GSV Base Time Unit : MIN

Special GSV Base Volume Unit : Standard cubic feet

Special GSV Conv Factor : 1

Special GSV Flow Unit Text : NONE

Special GSV Total Text : NONE

Special Mass Base Unit : G

Special Mass Conv Factor : 1

Special Mass Flow Text : NONE

Units

Special Mass Time Unit : SEC

Special Mass Total Text : NONE

Special Volume Base Unit : L

Special Volume Conv Factor : 1

Special Volume Flow Text : NONE

Special Volume Time Unit : SEC

Special Volume Total Text : NONE

Temperature Unit : C

Volume Flow Unit : L/MIN

MVD Channel Assignments

Channel B Power : Active (internally powered)

Assignments

Event 1 Variable : Density

Event 2 Variable : Density

Frequency1 Scaling Method : Frequency = Flow

Frequency Variable 1 : Mass Flow Rate

mA1 Variable : Mass Flow Rate

Ranges

Event 1 Setpoint : 0

Event 1 Type : Event Low (Event "OFF" if PV > SP)

Event 2 Setpoint : 0

Event 2 Type : Event Low (Event "OFF" if PV > SP)

Frequency1 Active State : Active High

Frequency1 Hertz : 1000

Frequency1 Output Mode : Single

Frequency1 Pulses/Unit : 1.554404

Frequency1 Rate : 643.3333

Frequency1 Units/Pulse : 0.64333333

mA1 LRV : 0

mA1 URV : 643.3333

Faults

Frequency1 Fault Behavior : Upscale

Faults

Frequency1 Fault Value : 15000
mA1 Fault Behavior : Downscale (Default)
mA1 Fault Value : 2

Other

Calibration Process ID : 9.29601901

Core Software Rev : 35
Density Cutoff : 0.2
Density Damping : 1.6
Density High Limit : 5
Density Low Limit : 0
Direction : FORWARD
Fault Dwell Time : 0
Feature Key : 1
Flow Damping : 0.8
HART Device ID : 4133198
LD Type : 0
Mass Flow Cutoff : 1.836
Pressure Comp Line Pressure : 0
Pressure Compensation State : OFF
RS485 Baud : 1200 baud
RS485 Parity : Odd
RS485 Protocol : HART
Slug Duration : 0
Tag :
Temperature Damping : 4.8
Transmitter Software Rev : 80
Volume Flow Cutoff : 0.11016

22081332