

Product Code

CNG050S290NCAAEEZZZ

Serial ID

15329813

26172485

Order ID

10507915

Line

2.1

Item

2

Customer Tag

2304/417

Process



Process ID : 1.36988786

Process Time : 2022.10.10 10:57:59

Process Stand : TSM1C@SSCB:1

Stand Uncertainty : +/-0.030%


Fluid : H2O

100% Rate : 38.6 KG/MIN

Pickoff : 1

Max Rate P/T : 29.79 PSIG/22.4 C

Detail

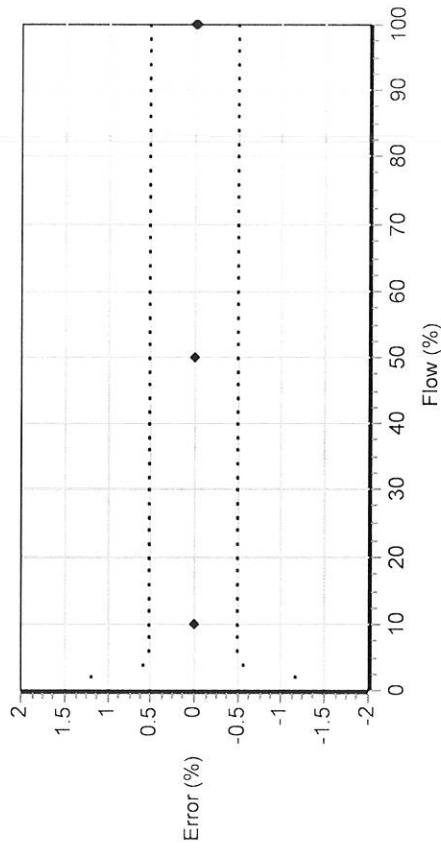

Results

Status : PASS

D1 : 0

D2 : 1

K1 : 4048.502

K2 : 4214.476

DT : 4.25

FD : 0

DTG : 0

DFQ1 : 0

DFQ2 : 0

FlowCal : 141.524.50

FFQ : 0

FTG : 0

DensCal : 04049042144.25

FCF : 141.52

FT : 4.5

Flow (%)	Flow Rate (kg/min)	Meter Total (kg)	Reference Total (kg)	Error (%)	Specification (±%)
100.0	38.6	39.5695	39.57827	-0.022	0.500
10.0	3.86	5.621511	5.621294	0.004	0.500
50.0	19.3	19.17101	19.17076	0.001	0.500
100.0	38.6	39.54827	39.54665	0.004	0.500

[Signature]
 DANG, HUONG N.
 Technician

This certificate is produced by an electronic data system and is valid without signature.

Product Code

CNG050S290NCAAEZZZ

2700I13ABAEZMZ

PUCK700

Serial ID

15329813

12221721

26172485

Order ID

10507915

10507915

Line Item

2.1 2

2.33 2

Customer Tag

23041417

Process

Process ID : 1.36989297

Process Time : 2022.10.10 14:18:39

Process Stand : CONFIGURATION@SSCB

Sensor

D1 : 0

D2 : 1

DFQ1 : 0

DFQ2 : 0

DT : 4.25

DTG : 0

Dens PCF : 0

Density Meter Factor : 1

FCF : 141.52

FD : 0

FFQ : 0

FT : 4.5

FTG : 0

Flow PCP : 30

Flow PCF : 0

K1 : 4048.502

K2 : 4214.476

Mass Flow Meter Factor : 1

Volume Flow Meter Factor : 1

Units

Special Mass Time Unit : SEC
Special Mass Total Text : NONE
Special Volume Base Unit : L
Special Volume Conv Factor : 1
Special Volume Flow Text : NONE
Special Volume Time Unit : SEC
Special Volume Total Text : NONE
Temperature Unit : C
Volume Flow Unit : L/MIN

MVD Channel Assignments

Channel B Power : Active (internally powered)

Assignments

Event 1 Variable : Density
Event 2 Variable : Density
Frequency1 Scaling Method : Frequency = Flow
Frequency Variable 1 : Mass Flow Rate
mA1 Variable : Mass Flow Rate

Ranges

Event 1 Setpoint : 0
Event 1 Type : Event Low (Event "OFF" if PV > SP)
Event 2 Setpoint : 0
Event 2 Type : Event Low (Event "OFF" if PV > SP)

Frequency1 Active State : Active High
Frequency1 Hertz : 1000
Frequency1 Output Mode : Single
Frequency1 Pulses/Unit : 1.554404
Frequency1 Rate : 643.3333
Frequency1 Units/Pulse : 0.6433333
mA1 LRV : 0
mA1 URV : 643.3333

Faults

Frequency1 Fault Behavior : Upscale

Units

Density Unit : G/CM3
GSV Flow Unit : SCFM
Mass Flow Unit : G/SEC
Pressure Unit : POUNDS/SQUARE INCH
Special GSV Base Time Unit : MIN
Special GSV Base Volume Unit : Standard cubic feet
Special GSV Conv Factor : 1
Special GSV Flow Unit Text : NONE
Special GSV Total Text : NONE
Special Mass Base Unit : G
Special Mass Conv Factor : 1
Special Mass Flow Text : NONE

Faults

Frequency1 Fault Value : 15000
mA1 Fault Behavior : Downscale (Default)
mA1 Fault Value : 2

Other

Calibration Process ID : 1.36988786
Core Software Rev : 35
Density Cutoff : 0.2
Density Damping : 0.8
Density High Limit : 5
Density Low Limit : 0
Direction : FORWARD
Fault Dwell Time : 0
Feature Key : 1
Flow Damping : 0.8
HART Device ID : 6220326
LD Type : 0
Mass Flow Cutoff : 1.836
Pressure Comp Line Pressure : 0
Pressure Compensation State : OFF
RS485 Baud : 1200 baud
RS485 Parity : Odd
RS485 Protocol : HART
Slug Duration : 0
Tag :
Temperature Damping : 2.4
Transmitter Software Rev : 80
Volume Flow Cutoff : 0.11016

23041417



Tulsa Gas Technologies, Inc.
4809 S. 101st East Ave Tulsa, OK 74146
PHONE: 918-665-2641 FAX: 918-665-2657

5/15/2023

Dispenser Serial Number 23041417

Micro Motion Transmitter Configuration

Required settings for correct operation of Micro Motion mass flow meter.

Transmitter Model Number: 2700
Sensor Model Number: CNG050
Transmitter Serial Number 12221721
Sensor Serial Number 15329813
Flow Calibration Factor: 141.524.50
Flow Units LB/min

Communication on RS-485

Protocol Modbus ASCII 7 Bit
Modbus Address 1
Baud Rate 9600
Parity Even
Stop Bits 1

HART Communication

Superimposed on Primary mA (PV)

Analog Output (4-20 mA)

Analog Variable (PV) Mass Flow
Lower Range Value 0.2500 lb/min
Upper Range Value 300.000 lb/min
mA Cutoff 0.0000 lb/min

Freq/Rate

Frequency variable (TV) Mass Flow
Frequency Cutoff 0.2500 lb/min
Pulses per Unit 1000.00000 per lb

Temperature

Temp Units deg F